



# Base Fortessa 2-B 3-R 5-V 3-UV 5-YG

Cytometer:	LSRFortessa	User:	Administrator
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 9.0
Input Device:	Manual	Date:	2/17/2023 8:54:44 AM
Window Extension:	10.00		


Blue Laser  
(488nm)  
FSC

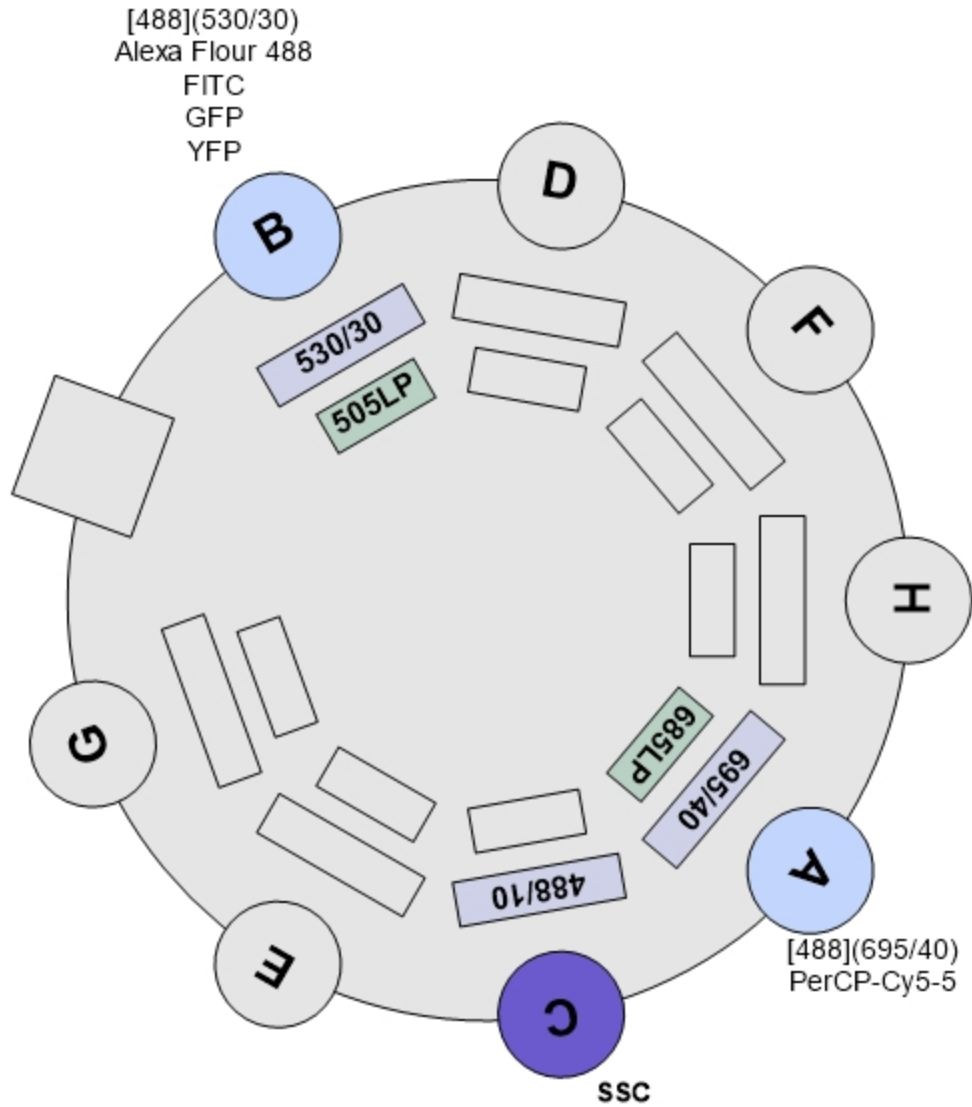


Red Laser  
(640nm)

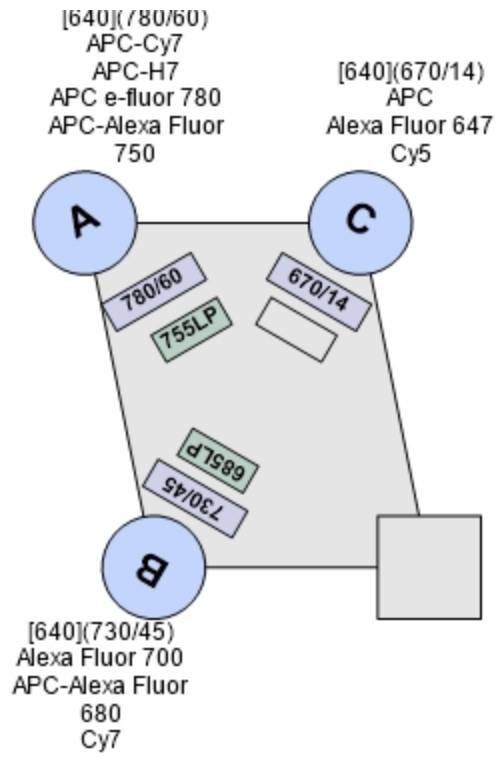


Violet Laser  
(405nm)

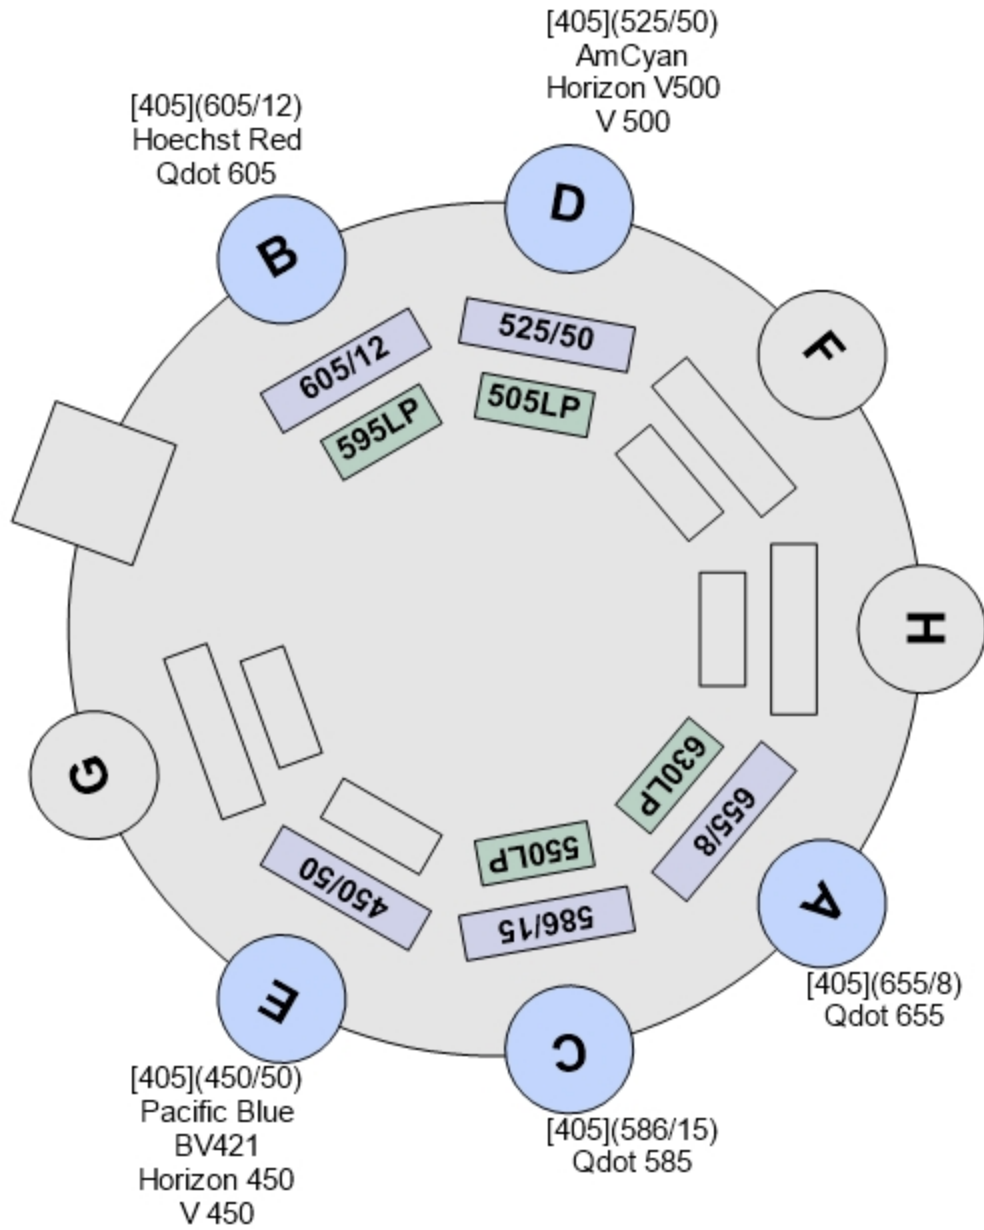

UV Laser  
(355nm)

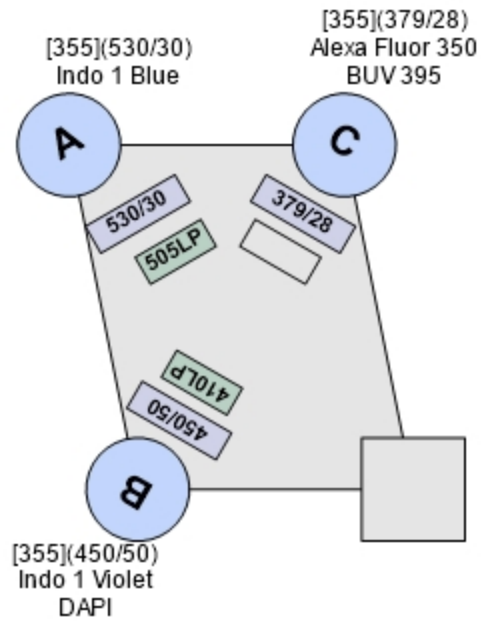

Yellow\_Green Laser  
(561nm)

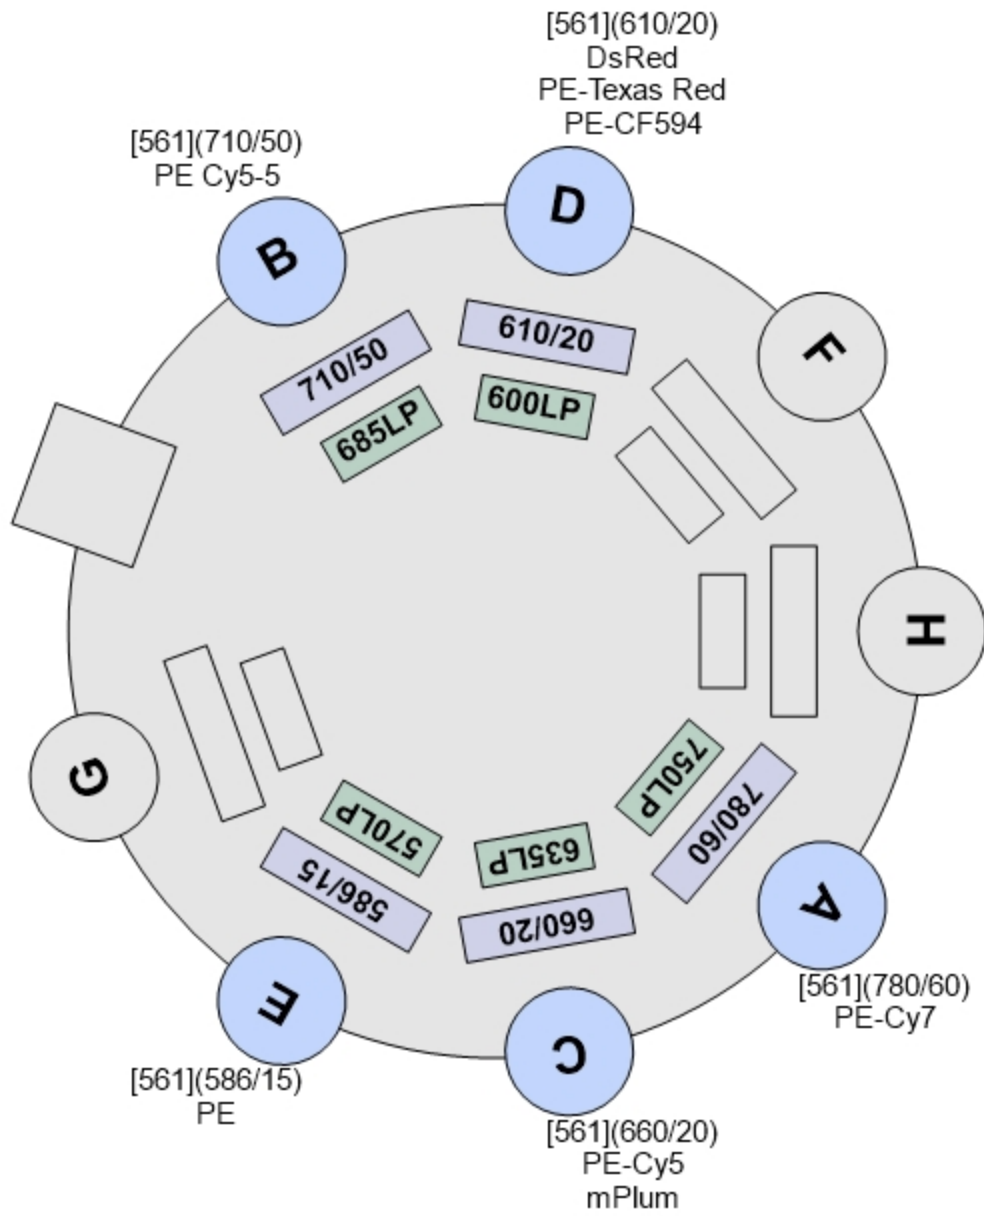

Comments: